

# Certificate of testing

## Crash Test according to ISO 10542-5 & 7176-19 - 2008

### Wheeled mobility devices for use in motor vehicles

This report serves solely as documentation for the test results. The tested objects have been selected by the client with out the assistance of Dahl Engineering.

**Assignment:** Crash testing of wheel chair and WTORS according to ISO 10542-5 & 7176-19

**Date of testing:** 28/4 2011

**Test object:** TA Indoor Wave wheelchair

**Mass of wheelchair:** 115 Kg

**Serial no:** 0174

**WTORS:** Wheelchair restraint system – Dahl Docking Station  
Occupant restraint – Dahl 3p. static shoulder and lap belts  
Systems meet requirements set out in ISO 10542

**Test dummy:** The test was carried out using a Hybrid II 50% dummy with mass of 76 Kg.

**Measuring:** The deceleration was measured by accelerometers mounted on the crash test sled.

**Photografi:** The test was filmed with a high speed camera at 500 fps.  
Still pictures, pre and post test, was also taken.

### Test results

**Sled deceleration and speed:** See page with plotted graph and speed

## Test Results

| Section      | Details   | X if correct |
|--------------|---|--------------|
| <b>5.21</b>  | <b>During the test</b>  |              |
| (a)          | Horizontal excursion limits   |              |
|              | Wheelchair point P $\leq$ 200 mm [Xwc]  | 81           |
|              | ADT knee $\leq$ 375 mm[Xknee]   | 169          |
|              | ADT front of head $\leq$ 650 mm [XheadF]  | 272          |
|              | ADT rear of head $\leq$ - 450 [XheadR]  | -234         |
| (b)          | The knee excursion exceeded the wheelchair P point excursion  | X            |
| (c)          | (Batteries on powered wheelchairs) did not move completely outside the wheelchair footprint or move into the wheelchair user's space or contact with ADT legs | X            |
| <b>5.2.2</b> | <b>After the test</b>   |              |
| (a)          | The wheelchair remained in an upright position on the platform  | X            |
|              | The ADT remained in the wheelchair with its torso at an angle of not more than 45° to the vertical, when viewed from any direction                            | X            |
| (b)          | There were no visible signs of material failure on the wheelchair securing points   | X            |
| (c)          | There were no components, fragments or accessories of the wheelchair with a mass of more than 100g that completely separated from the wheelchair              | X            |
| (d)          | There were no fragmented or separated component, that may contact the occupant, produced with sharp edges less than radius 2 mm                               | X            |
| (e)          | There were no visible signs of failure on the wheelchairs primary load carrying components  | X            |
| (f)          | There were no visible signs of failure on the wheelchairs seat adjusters  | X            |
| (g)          | The ADT was removed from the wheelchair without the use of tools  | X            |
| (h)          | The wheelchair was released from the tie-down system without the use of tools   | X            |
| (i)          | The post test decrease of the mean H-point height is not more than 20%  | X            |
| (j)          | Wheelchair and components did not cause partial or complete failure of the webbing of any of the WTORS assemblies during the test                             | X            |

The presented samples meet the requirements set out in the above mentioned standard.

### Test Laboratory:

Dahl Engineering - Research and Testing Laboratory  
Løvevej 3 - DK-7700 Thisted - Denmark  
Phone: 45 96180077 - Fax: 45 96180078  
e-mail: [Dahl@dahlengineering.dk](mailto:Dahl@dahlengineering.dk) – web page: [www.dahlengineering.dk](http://www.dahlengineering.dk)

Thisted 28 April 2011



Claus Dahl Pedersen  
Head of test laboratory


Plotted graph and speed



**SLED - TEST**  
Project: TA Service


|  |   |
|--|---|
| Editor: NG                               | Specification: ISO10542-5 / ISO7176-19        |
| Date: 04/28/2011                         | Test type: Homologation Test                  |
| File: TA Service2011-032                 | Test structure: TA Service Indoor Wave        |
| Sensors: ASC 4311 400 g, S/N-Nr.:G 81289 | Test sample: Dahl Docking Station             |
| Measurement: A/D Karte, DT 321           | Comment to sample: WC weight 115 kg           |
| Analysis Sequence: Standard              | Occupant: HybridII 50% Male                   |
| Sled velocity: 48.5 km/h                 | General comment: Dahl 3 p. occupant restraint |

**SLED ACCELERATION**

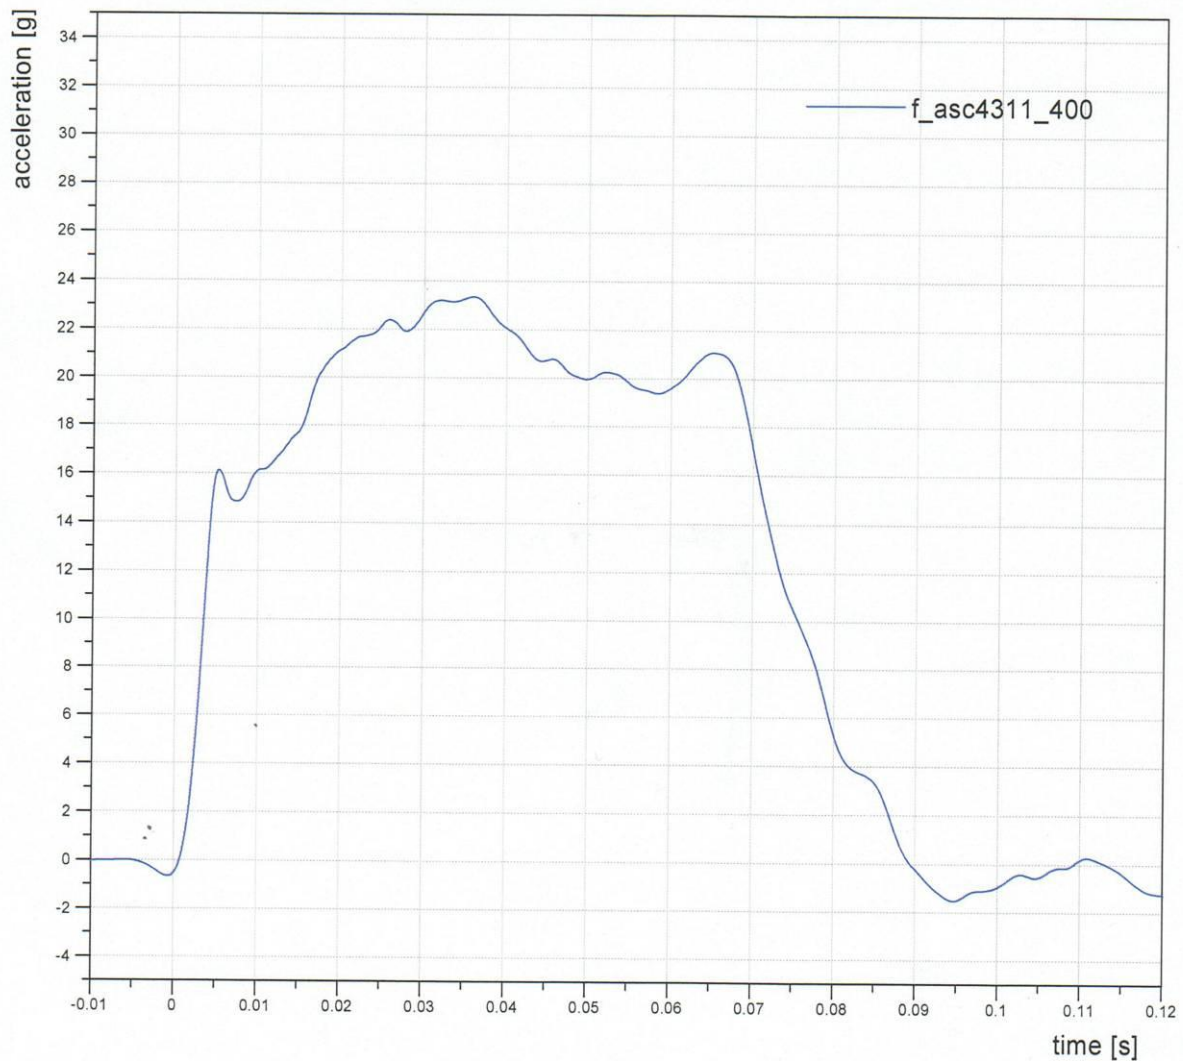




Pre- test photos

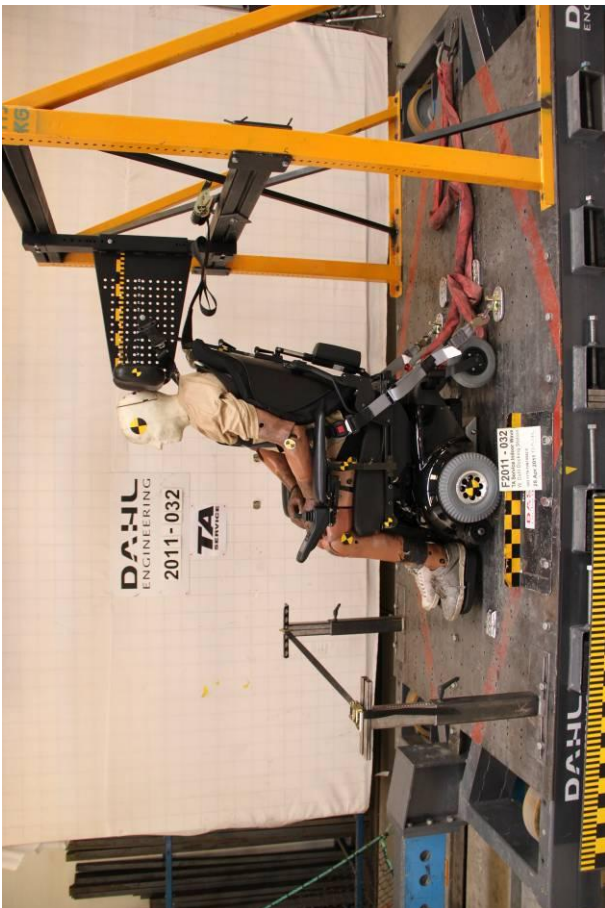



Post test photos

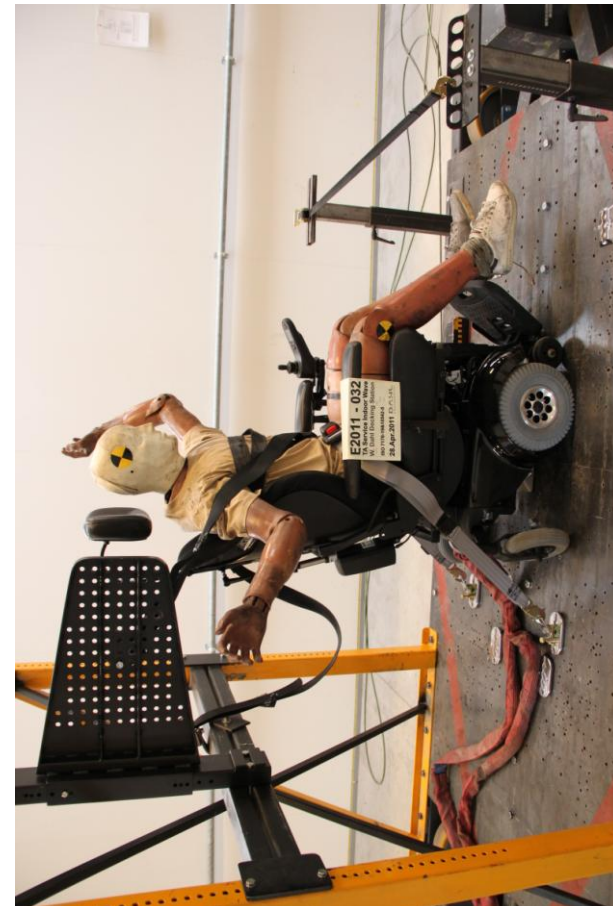



Post test photos

